


EM=516

LCMS Scan ESI+

Ret. Time: 2.06

<<<< POSITIVE SPECTRA >>>>

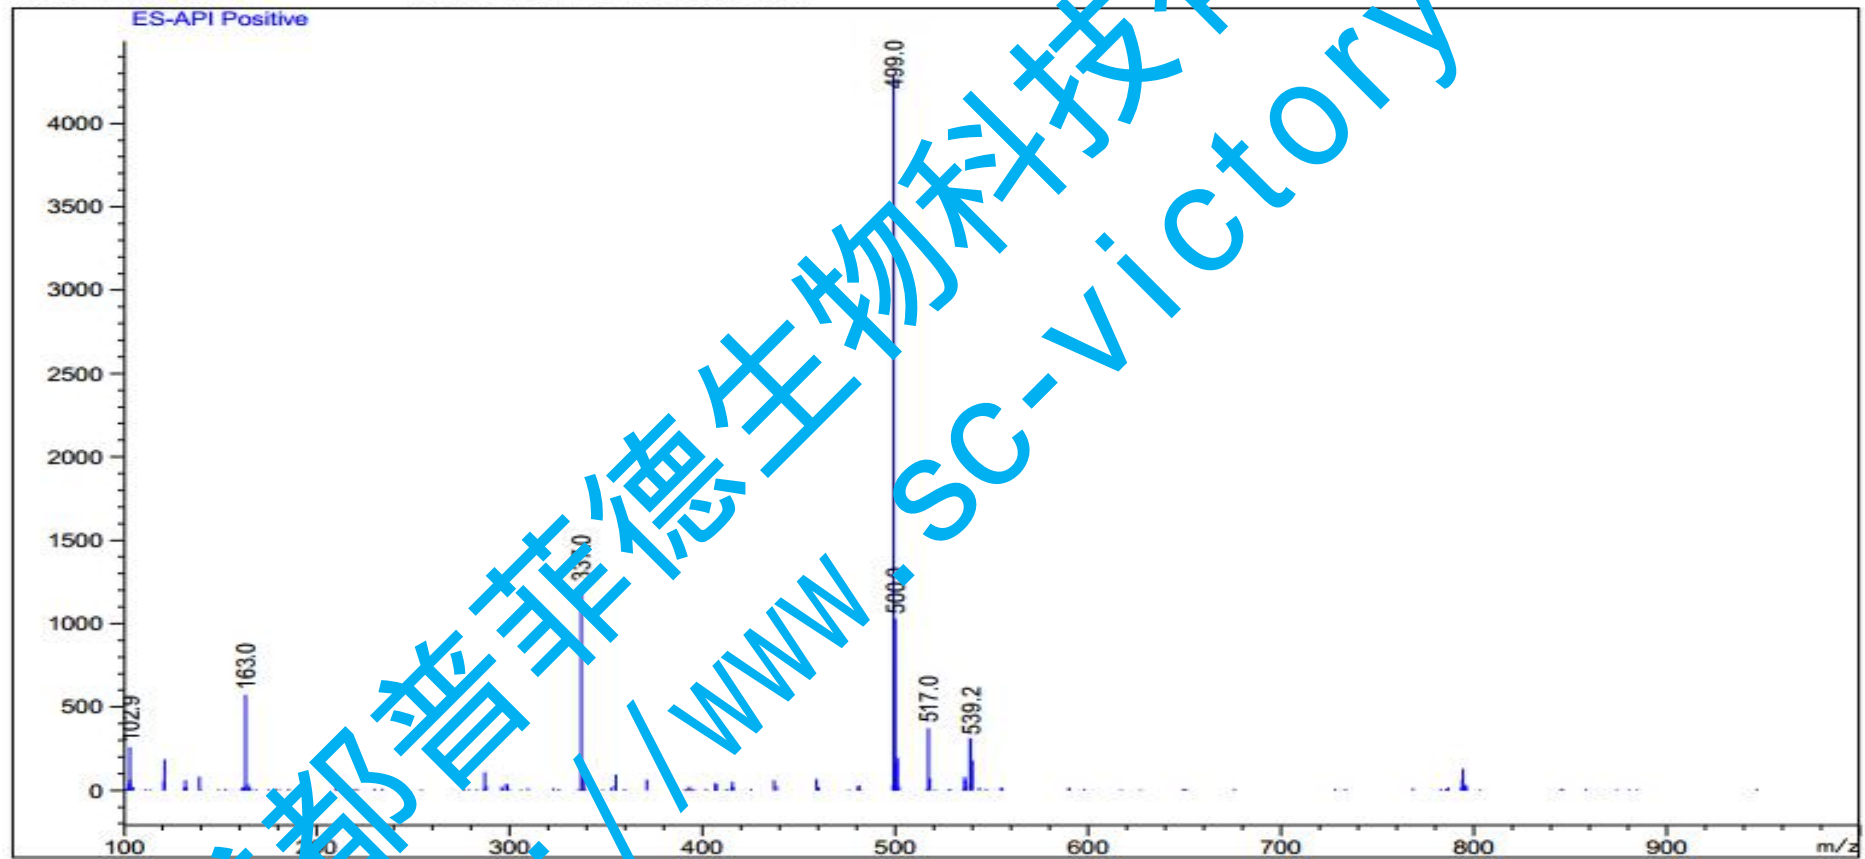


成都普菲德生物科技有限公司
http://www.sc-victory.com

EM=516

LCMS Scan ESI-

Ret. Time: 2.07

<<<< NEGATIVE SPECTRA >>>>

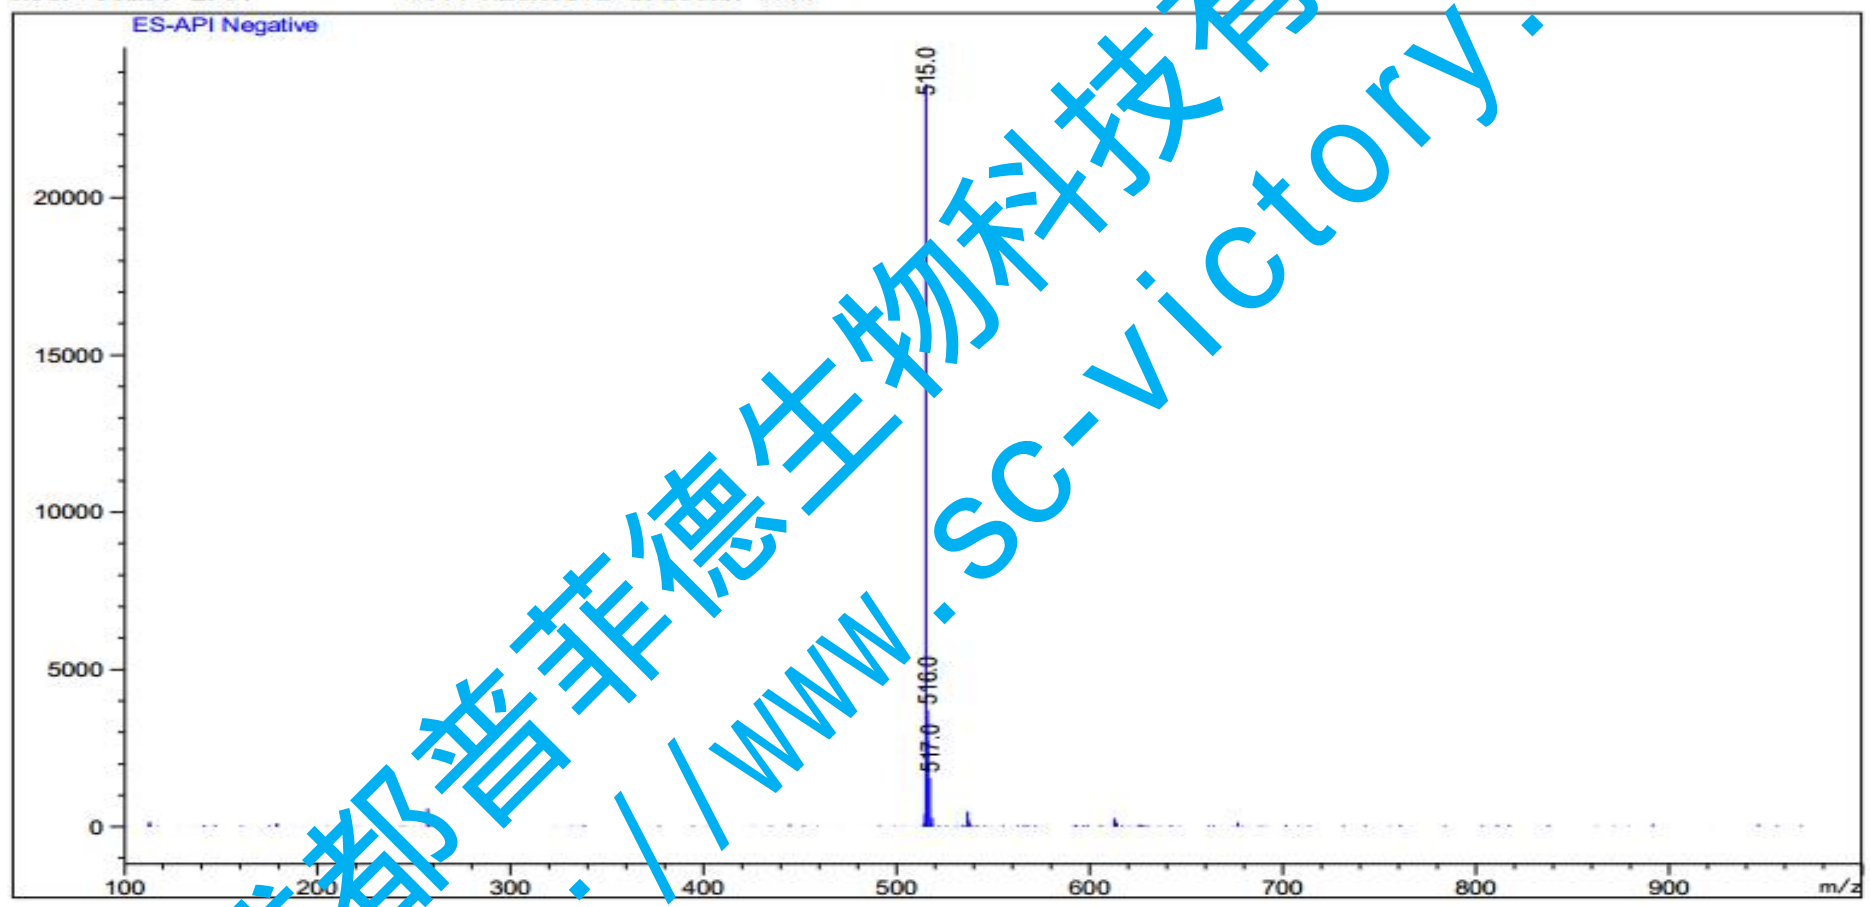

成都普菲德生物科技有限公司
http://www.sc-victory.com