


EM=610

LCMS Scan ESI+

Ret. Time: 0.52 <<<< POSITIVE SPECTRA >>>>

F

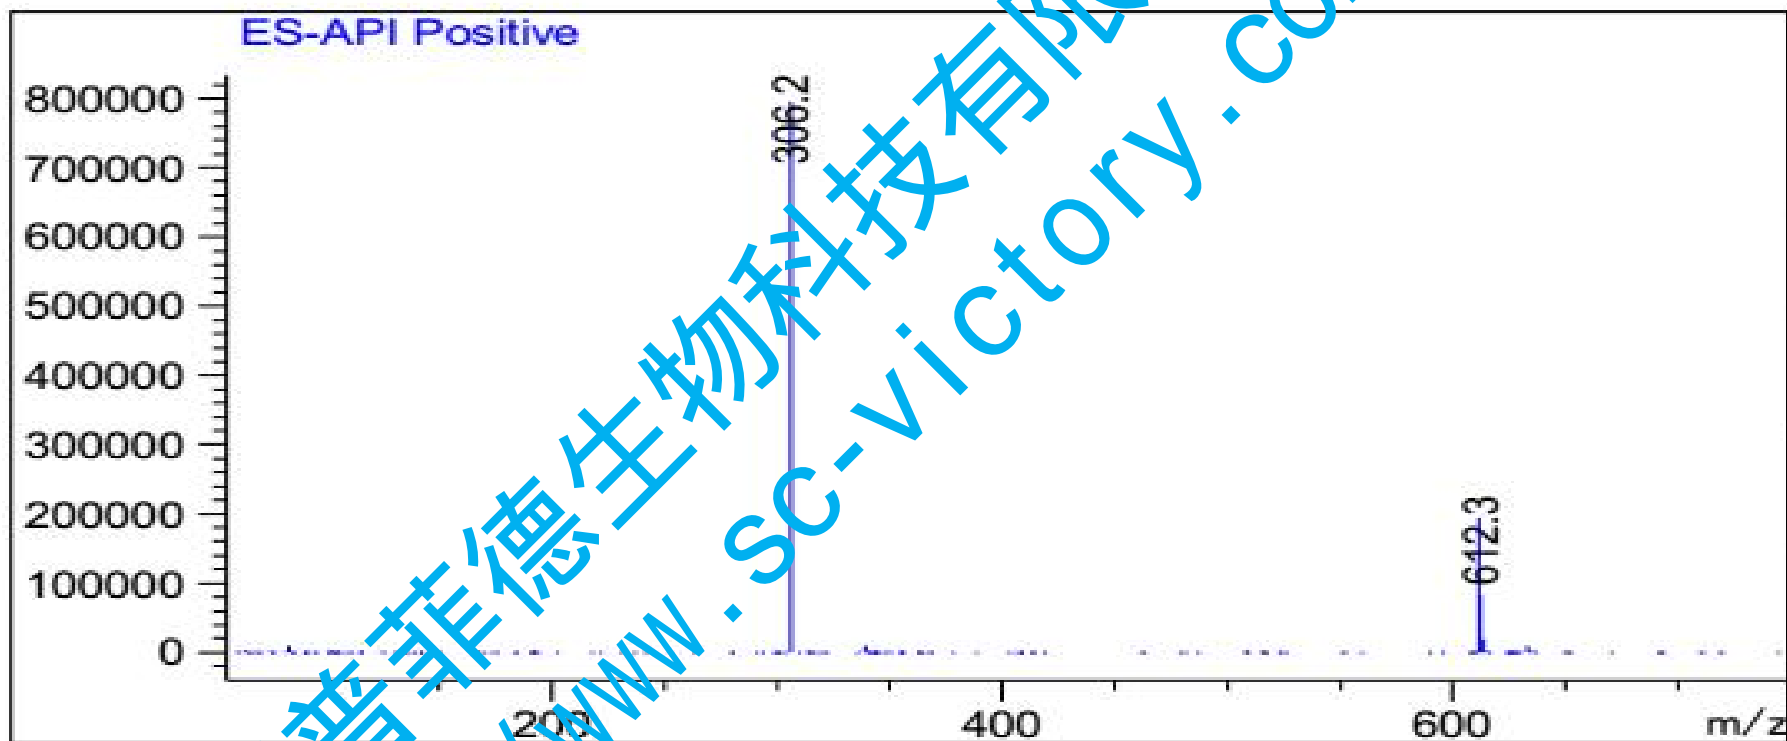


成都普菲德生物科技有限公司  
<http://www.sc-victory.com>

EM=610

LCMS Scan ESI-

Ret. Time: 0.56 <<<< NEGATIVE SPECTRUM >>>> F

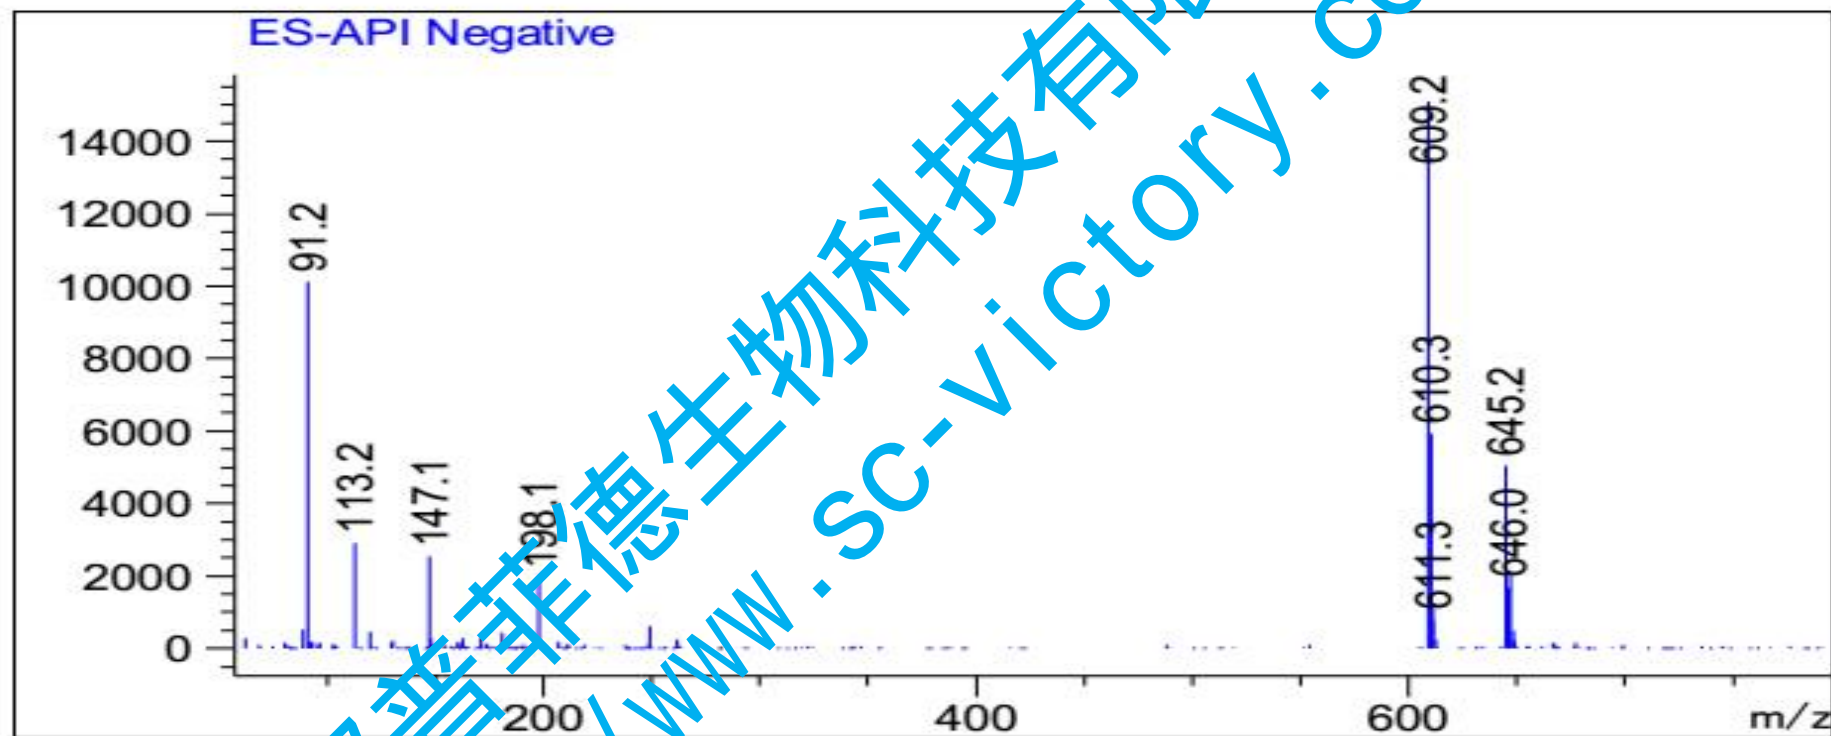

成都普菲德生物科技有限公司  
<http://www.sc-victory.com>